

# HILO THERM<sup>®</sup>

## *ChemoCare-CIPN*

### Instructions for use



CE 0123



**HILO THERM GmbH**  
Wittumweg 38  
D-88260 Argenbühl Iron Resin  
Phone +49 / 75 66 / 9 11 99

# Table of contents

## **1.General description**

- 1.1 Purpose
- 1.2 Usages of application
- 1.3 Indications and contraindications
- 1.4 Requirements for operators
- 1.5 Device description

## **2.Safety instructions**

- 2.1 General safety instructions
- 2.2 Hazard warnings
- 2.3 Electromagnetic compatibility
- 2.4 Environmental conditions

## **3.Commissioning**

- 3.1 Functional control
- 3.2 Establish
- 3.3 Operation and after water change
- 3.4 Filling and switching on
- 3.5 Set temperature
- 3.6 Connecting the cuffs
- 3.7 Ending
- 3.8 Failures
- 3.9 Menu

## **4.Cleaning and disinfection**

- 4.1 General
- 4.2 Device surface
- 4.3 Cots

## **5.Maintenance, inspection**

- 5.1 Replace water filters and change water
- 5.2 Cleaning heat exchangers
- 5.3 Grease plug connections
- 5.4 Review
- 5.5 Safety control
- 5.6 Liability
- 5.7 Warranty

## **6.Storage, transport, disposal**

- 6.1 Storage
- 6.2 Transport
- 6.3 Displacement

## **7.Technical data**

- 7.1 Technical data
- 7.2 Characters
- 7.3 Security standards
- 7.4 Discussions and troubleshooting

## **8.Accessories and spare parts**

- 9.1 Variants and material properties
- 9.2 Warning notes
- 9.3 Product use
- 9.4 Risk classification
- 9.5 Application description
- 9.6 Storage, storage and Transport
- 9.7 Defection, cleaning and
- 9.8 Control and testing
- 9.9 Packaging
- 9.10 Sterilization

## **10.Annex**

- A guidelines and manufacturer's declaration
- B declaration of conformity



Before commissioning the Hilotherapy system, the instructions for use must be read. Pay particular attention to **the caution** and **warning** instructions.

Caution describes a situation in which the device or connected modules can be damaged.

**Caution/** Warning describes a situation in which people may be harmed. Increased attention and care should be applied.

## 1. General description

### 1.1 Purpose

HILOTHERAPIE using the Hilotherm ChemoCare System is a form of physical thermotherapy that uses a constant temperature in the range of 5°C to 25°C locally. Applications lasting several hours can be carried out without temperature deviations. Used prophylactically, HILOTHERAPY with ChemoCare significantly reduces the risk of **chemotherapy-induced polyneuropathy** (CIPN) – also known as **hand-foot syndrome** (HFS).

#### Principle of action:

In chemotherapy, parts of the chemotherapy drug are directed via the sweat glands to the surface of the skin, where "free radicals" form in contact with oxygen. These damage the tissue cells of the skin, especially where it is particularly thick as a cornea and absorbs the substance like a sponge >> on the palm and sole of the foot.

To prevent the chemotherapy drug from penetrating into the capillaries of the extremities, it is necessary to slow down blood circulation and metabolism. This is done by lowering the tissue temperature.

With the Hilotherapy system Hilotherm ChemoCare consisting of the temperature control devices "as well as hand and foot cuffs, the tissue temperature is locally adjusted in the area of hands and feet to an individual value prescribed by the doctor and kept constantly cool.

The therapy device with the cuffs and connection tubes forms a closed circulatory system through which the cooling medium flows and keeps the set temperature constant.

### 1.2 Areas of application

Thermotherapy with the "Hilotherm ChemoCare" is used prophylactically before and during chemotherapy to reduce the risk of chemotherapy-induced polyneuropatia.

#### **Duration of use**

The use of thermotherapy should be carried out half an hour before the start of therapy and during chemotherapy.

### 1.3 Indications and contraindications

#### **Indications for hilotherapy**

Indication for hilotherapy (localized lowering of tissue temperature) is chemotherapy-induced polyneuropathy (CIPN)

A common complication of chemotherapy with certain cytostatic drugs, such as B. carboplatin, capecitabine, 5-Fu, cyclophosphamide, cytarabine, docetaxel, doxorubicin, oxaliplatin, paclitaxel, sorafenide and sunitinib, is hand-foot syndrome.

This refers to side effects on the hands and feet that can occur both shortly after the start of chemotherapy or only in the course or months later.

The symptoms are: numbness in the hands and feet with gait uncertainty, decrease in tactile sensation, loss of depth sensitivity, loss of temperature perception, burning pain, disturbance of coordination as well as hypersensitivity of the skin, e.B. when touched.

## Contraindications to hilotherapy

**Contraindicated are all forms of cold applications in the presence of cryoglobulinemia, cold hemagglutination and cold urticaria / cold contact urticaria caused by histamine release.**

Hilotherapy is also not indicated for diseases in the area of functional circulatory disorders (e.B.M. Raynaud's disease), severe arterial occlusive disease, pronounced sensitivity disorders and trophic tissue lesions.

## 1.4 Requirements for operators

The operation of the Hilotherapy device is simple and can be carried out by nursing staff or the patient himself. However, the application should be supervised by qualified medical personnel.

Before commissioning, the instructions for use must be known and the operator must familiarize himself with the device. In particular, the application of the cuffs must be done carefully.

## 1.5 Device description

The Hilotherapy System HT 02-c is a transportable system for local professional cold treatment. It consists of 2 cooling units, a transport trolley and corresponding cuffs for hand and foot cooling.

It is characterized by its easy handling and easy operation.

The temperature is adjustable from + 5°C to 25°C

The device is intended for continuous operation.


The Hilotherapy cooling unit essentially consists of the following components:

**Cooling unit** With the cooling unit, distilled water is tempered to the exact degree and kept constant.

**Control** The controller records the data in the device via sensors and regulates all processes. With the keys (item 04) the desired value for the temperature is entered.

**Display** The display (item 03) shows the set values and the operating status.

**The following describes the use of a cooling unit of the ChemoCare system. The two cooling units of the HILOTHERM ChemoCare System are identical and can therefore be operated in the same way.**

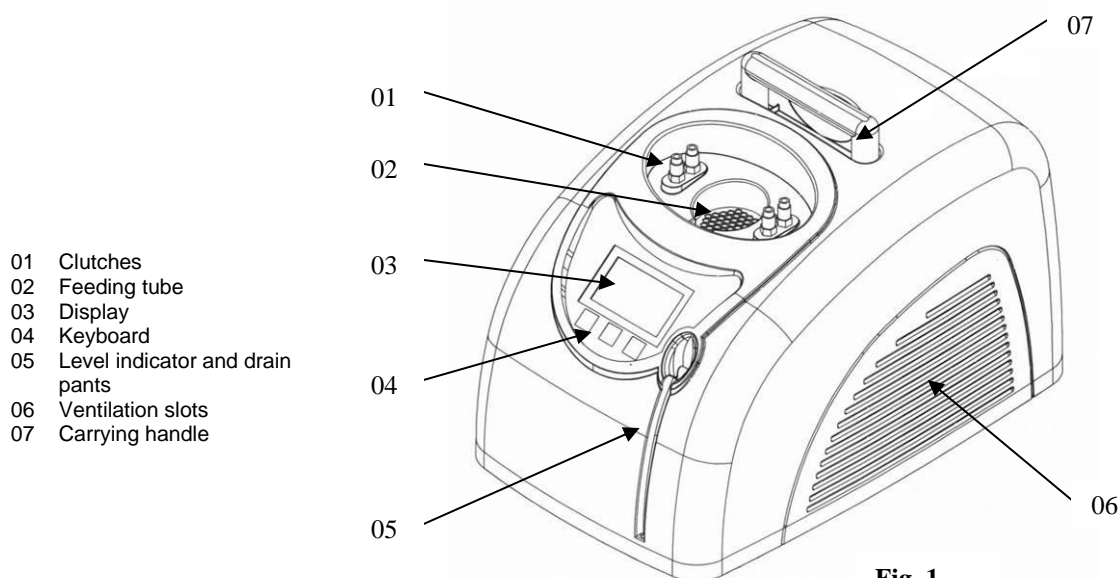

## 2. Safety instructions

### 2.1 General safety instructions

- Before commissioning, the user must check the correct condition of the device and user part.
- The therapy facility always consists of the Hilotherapy device, connecting tube and cuff(s).
- Only original Hilotherapy devices and cuffs may be connected and used.
- When switched off, the good thermal conductivity of water can lead to an unwanted change in body temperature in large cuffs (cooling when applying heat, heating when applying cold).
- If the intended use cannot take place due to malfunctions, the cuff must be removed.
- During application, especially when using several or large cuffs, the patient's body temperature should be monitored.
- The hilotherapy system must not be operated in the incubator.
- The cuffs can be damaged by the penetration of sharp objects.
- The flow of the channels in the cuffs can be prevented by folding the cuffs or by pressing.
- The flow of the hoses can be prevented by buckling.
- The tank may only be filled with demineralized water.
- When filling with demineralized water, the power plug must not be plugged in.
- The lateral ventilation slots must not be closed or covered. The device may only be operated in a horizontal position on a fixed flat surface.
  
- The device must not be put into operation if not all aggregates and displays are working properly.
- In the event of malfunctions, the device must be switched off immediately. It may only be used again when the fault has been resolved. In the event of critical or unclear errors, the manufacturer must be notified.
- Interfaces for the service area and data exchange must not be used when a patient is connected to the device.
- **Warning:** Changing the device is not allowed

### 2.2 Hazard statements

- The housing must not be opened.
- Before carrying out maintenance measures, the device must be disconnected from the power supply.
- Maintenance may only be carried out by qualified service technicians.
- The AC voltage source shall correspond to the specified range located on the nameplate on the back of the device.
- The Hilotherapy system may only be connected to mains voltages connected to a reliable protective mass conductor. Do not use the system if the functionality of the external, protective mass conductor is questionable.
- In order to ensure fire protection, care must be taken when replacing the fuses that only fuses of the same type and with the same nominal values are used (see type plate).

### 2.3 Electromagnetic compatibility

In the case of medical electrical equipment, special attention must be paid to electromagnetic compatibility (EMC). This means that the devices must be installed and put into operation in accordance with the EMC instructions contained in these operating instructions (see instructions and manufacturer's declaration in the annex).

Portable and mobile radio communication equipment can affect medical equipment.

**Warning:** The Hilotherapy system should not be operated alongside/on other equipment. Should this be necessary, the hilotherapy system must be monitored to ensure safe operation.

### 2.4 Environmental conditions

The ambient temperatures for safe operation are between + 10 °C and + 26 °C.

At higher temperatures, the guaranteed cooling capacity cannot be provided. If the device has been exposed to temperatures that are far outside the specified temperature range, it should be waited before commissioning until the device has reached room temperature.

The humidity in the room should not exceed 70%. Higher humidity can lead to condensation on the hoses and cuffs.

**Caution:** Accumulation of condensation can lead to a risk of slipping on the floors. If this is detected, appropriate security measures must be initiated

Protect the device from excessive heat, dust and direct sunlight.

**Warning:** The Hilotherapy system is not intended for operation in highly explosive environments and must be kept away from flammable gases and liquids.

## 3. Commissioning

### 3.1 Functional control

Before commissioning the Hilotherapy system, devices and user parts must be checked for damage (see Chapter 2. Safety instructions).

**Caution:** The system may only be put into operation if all components are undamaged.

### 3.2 Installation

- The Hilotherapy system with trolley set up on a horizontal, flat, hard surface.
- These devices must be set up in such a way that air circulation is not impeded.
- A minimum distance of 20 cm on the side and 10 cm on the top must be maintained to other devices or furniture.
- The system must be set up in such a way that disconnection from the power grid is not made more difficult.
- Make sure that the device vents are not directed at the patient.

### 3.3 Initial commissioning and after water change

Attention: During initial commissioning and after water change, the pump system must be vented before switching on the Hilotherapy device.

- To vent, insert the vent syringe with the plug-in sleeve onto one of the front clutches.
- Pull out the air with the syringe.
- Remove the vent syringe.

**Caution:** During initial commissioning or after the water change, the device must only be switched on with the cuff connected so that the air can escape from the pump system and the pump does not run dry.


If the pump starts up and no water is pumped into the cuff, the pump must be vented again.

### 3.4 Filling and switching on


- Fill the water container with demineralized water. The level indicator should be located at the "max" marker.

**ATTENTION:** In the cold unit that supplies the **foot cuff of the 2nd generation**, the water level of the device must be filled exactly to the "max" mark before filling the cuffs.

Otherwise, the water level message "E21" appears and some water must be refilled (about 1 cm on the display scale). If there is too much water in the device, there may be an overflow in the filling funnel of the device after switching off the device and the

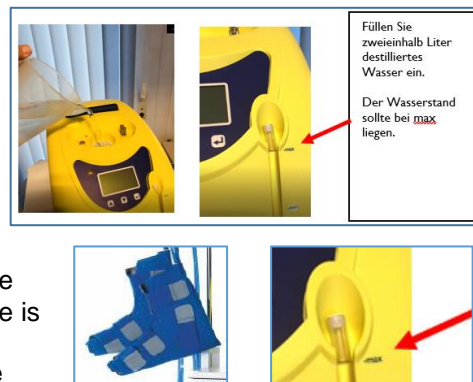

associated return from the cuffs.

- During initial commissioning and after water change, ventilate the pump system, see 3.3.
- Plug in the power plug.
- Turn on the device at the main switch on the back of the device. When switched on, the device checks itself. At the end of the self-test, an acoustic signal sounds and the menu appears on the display, see 3.9.
- Connect the connection hose and the cuff.
- Set the desired set temperature.
- Press the button. 
- Make sure that water is pumped through the cuff.



### 3.5 Setting temperature to cuff type

- The desired target temperature during the application is displayed on the display. Changed the arrow keys ▲ (for higher) and ▼ (for lower).
- The set value is automatically applied and the Hilotherapy device changes the actual temperature to the desired value.

For the cooling of the hands and feet, both first-generation cuffs (1st generation) and second-generation cuffs (2nd generation) can be used. Cuffs of the 2nd generation have the property of a more efficient cold transmission and thus achieve an even better CIPN prevention result. In addition, when using the 2nd generation cuffs, the set temperature can be set higher and thus more pleasant:

Cuffs of the first generation (1st generation)



Second generation (2nd generation) cuffs:




**The following device settings are recommended:**



### 3.6 Connecting the cuffs and hose attachment

- Cuff and connection hose are connected (audible snapping of the locking grommets into the couplings).
- The hose is plugged into the couplings with the locking grommets (Fig. 1).
- The swapping of feed and return is permissible and does not lead to malfunctions.
- When putting on, make sure that the cuffs are not placed over sharp edges or pointed objects.
- The uncoupling of the cuffs is carried out by retracting the gripping ring.

### 3.7 Exit

- Pressing the button terminates the operation. 
- At the main switch on the back, the device is switched off.
- If the device is not used for a long time, it must be disconnected from the supply network by unplugging the mains plug.

### 3.9 Faults

Disturbances are indicated by an optical and/or short acoustic signal.  
The cause of the disturbance is described in item 7.4.

### 3.10 Menu


#### Turn on the device

Main switch on  
Device cools / heats  
Pressure pump off



#### Device is in operation

Device cools  
Pressure pump running

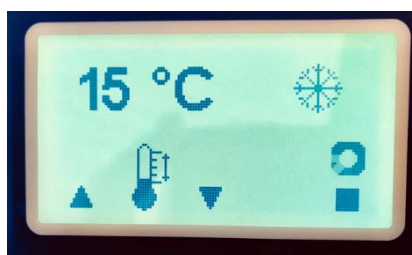


The temperature can be changed in both operating states.

**A flashing snowflake means that the device is in the cooling phase into the temperature target range. If the snowflake appears permanently, the cooling temperature of the device is in the target area.**

#### Device operation – exclamation point flashing quickly

The cooling temperature no longer COMES to the finish area  
For troubleshooting, see item 7.4.

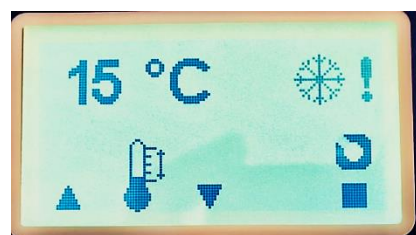



## Diagnosis

If an error occurs, the "E" indicator appears. Only the current error is displayed. The display can only be deleted when the error has been resolved.

**For troubleshooting and troubleshooting measures, see item 7.4.**



## 4. Cleaning and disinfection

### 4.1 General

**Caution:** The device must only be cleaned after it has been disconnected from the power supply. No sharp objects may be used for cleaning.

### 4.2 Device interface

Surfaces and equipment parts can be cleaned and disinfected with the usual and approved cleaning and surface disinfectants in the hospital sector.

Make sure that **no liquids get into the device**, especially through the vents on the sides.

### 4.3 Cuffs / user parts

Listed separately under point 9.7

## 5. Maintenance, inspection, safety control

The Hilotherapy system has been designed and manufactured to the highest quality standards.

When used as intended and carried out the intended maintenance and service measures, the device achieves a service life of 10 years and more.

In order to ensure the safety and functionality of the Hilotherapy system for a long time, the following maintenance measures must be carried out:

### 5.1 Replace water filters and change water – at least every 6 months

- Lift out the grid in the hopper with a small screwdriver.
- Remove the filter.
- Pull the hose of the water level indicator out of the guide on the housing.
- Remove the cover plug.
- Drain water completely.
- If necessary, rinse the tank with surface disinfectant (e.B. Kohrsolin FF or Mikrobac from Bode Chemie) and rinse with fresh distilled water.
- Push the drain hose back into the guide of the housing.
- Press in the cover plug.
- Insert a new filter.
- Place the grid back over the filter.
- Fill with demineralized water via the filling hopper, to which a preservative can be added.
- Vent the device (see point 3.3).

### 5.2 Clean heat exchangers – at least every 6 months or in case of visible contamination

Dust deposits on the heat exchanger reduce the cooling capacity of the device.

The heat exchanger is located behind the ventilation grille on the right side of the unit.

- Remove the three Phillips screws in the floor under the ventilation grille.  
*Caution:* The screws with hexagon socket must not be loosened!
- Remove the ventilation grille, carefully clean with a soft brush or vacuum cleaner.  
*Caution:* The cooling plates on the heat exchanger must not be damaged!

### 5.3 Grease plug connections – at least every 6 months

The plug connections of the hoses must be greased regularly so that they are easy to plug in and ensure complete locking of the locking grommets into the couplings.

- Thinly grease the tips of the closure grommets of the cuff and hose with petroleum jelly.
- Insert and unplug the closure grommets several times into the couplings of the hose or Hilotherapy device. The petroleum jelly is thus transferred to the O-rings in the couplings.

### 5.4 Inspection - at least every 2 years

Visual inspection:

- Is the instructions for use complete?
- Is the nameplate complete and legible?
- Are all markings and stickers on the device correct and legible?
- Are all parts fixed to the device (no parts loosened)?
- Is the housing undamaged?
- Are the connectors for the cuff connection smooth and undamaged?
- Do all switches and buttons work properly?
- Is the main backup in the device the specified type?
- To change the fuse, pull out the slot between the main switch and the device plug. After changing the fuse, press the slot until it clicks into place audibly.
- Is the device plug with main switch undamaged?
- Is the power cord undamaged?
- Are the device and accessories clean?
- Are the ventilation slots and the heat exchanger behind them clean?
- Is the accessory in perfect condition?
- Replace the water filter and distilled water.

Testing:

- Function of the cooling unit
- Function of the pressure pump (Are the cuffs sufficiently supplied?)
- Is wear and tear recognizable? (unusual noises?)
- Function of the water level sensor (error message water level when switching on with empty water tank?)

In addition, the following tests can be carried out

- Pressure testing
- Performance tests

In the event of detected defects, the device may not be used again until the defects have been remedied.

Maintenance measures may only be carried out by qualified personnel.

On request, the manufacturer supports the maintenance personnel through training and technical assistance. Info

### 5.5 Safety control

During production, a STK (safety inspection) is carried out as part of the final inspection.

In order to maintain operational safety, a new STK must be carried out when repair work has been carried out on the electrical system.

The operator is responsible for determining the scope of the test and the test interval (see §11 MPBetreibV). However, the STK must be carried out at the latest every 2 years at the end of the month.

## 5.6 Liability

HILOTHERM GmbH (as the manufacturer) is only liable for the effects on the safety, reliability and functionality of this device if:

- Assembly, extensions, new hires, modifications or repairs are carried out by authorized persons of the manufacturer.
- the parts and components used for repairs, modifications, extensions or local applications are approved by the manufacturer.
- the electrical installation to which the device is connected complies with the regulations of the local authorities.
- only the accessories approved by HILOTHERM GmbH are used.
- the device is used in accordance with the instructions for use.

## 5.7 Warranty

With regard to liability for material defects, the provisions of German law shall apply. This does not affect the statutory provisions of the Product Liability Act.

# 6. Storage, transport, disposal

## 6.1 Storage

The device should be stored dry and horizontally on flat ground, at a temperature of 5°C to 40°C and 10 – 70% RH and air pressure of 700 hPa – 1060 hPa.

**Caution:** If the device is stored below 0°C, the water of the cooling circuit must be completely emptied to avoid damage caused by freezing.

## 6.2 Transport

Before transport, the device must be completely emptied.

**Caution:** The device may only be transported on pallet with a forwarding agent, as horizontal transport is absolutely necessary.

## 6.3 Disposal (WEEE Reg.-Nr. DE 25202195)

The device must not be disposed of with general commercial or household waste.

In accordance with product responsibility according to § 22 of the Recycling and Waste Management Act and the Electronics Act § 2.2 paragraph 1, the device must be handed over to a corresponding municipal collection point or returned to the manufacturer.

When disposing of it, it should be noted that the appliance contains a refrigeration unit similar to a refrigerator (refrigerant: R134a).

**Warning:** There is oil in the compressor unit.

# 7. Technical data

## 7.1 Technical data

### Type HT02 *ChemoCare-CIPN*

Article No.	2020 0012
Rated voltage	230 VAC 50 HZ
Power consumption	max.320 VA
Current consumption	2.5 A
Fuse value	2.5 A 250 V
Protection class	I
Degree of protection application	part B
Protection class	IP 20
Risk class (93/42 EEC)	Ila

Dimensions	430 mm x 275 mm x 268 mm
Weight	10 kg
Cuff connections	2
Capacity water tank	min.1.25 liters, max. 2.25 liters
Temperature range	+ 5°C to + 25 °C
Control/setting tolerance	± 1°C

#### Refrigeration unit

Rated voltage	230 V 50 HZ
Working pressurePü zul.	25 bar intrinsically safe
Refrigerant	R 134a
	Capacity100 g

#### Positive displacement pump

Rated voltage	15 V
Operating pressure	0.5 bar +0.1

#### Heating

Rated voltage	230 V
Power consumption	220 VA

#### Ambient conditions

Storage temperature	minimum. + 5 °C, max. + 40 °C
Humidity storage	10 - 70% RH non-condensing
Operating humidity	10 - 70% RH non-condensing
Operating ambient temperature	+ 10 °C to + 26 °C

## 7.2 Characters

The following characters can be found on the device and on the packaging:



Follow the instructions for use  
see accompanying documents (instructions for use)



Manufacture  
(YYYY)



Device type B  
(Protection against electric shock)



CE marking for conformity according to EU Directive 93/42/EEC  
Medical devices with marking of the certification body



not for reuse /  
Use only once




do not dispose of general commercial or  
household waste



General warning sign. The device calls physiological effects  
(temperature changes) that are not obvious to the operator  
are.



Filling device, demineralized water filling



Drain device

### 7.3 Safety standards

#### Classification

According to the classification criteria in Annex IX EC Directive 93/42 EEC, the hilotherapy system is to be classified in **Class IIa Rule 9** (Active medical device for therapeutic purposes).

According to **the GMDN** classification, the device is assigned to **No. P 42463**, the Cuffs **No. P 44604**.

The Hilotherapy system is neither assigned to Appendix 1 and 2, **nor to Appendix 3** of the MPBetreibV.

#### Standards and guidelines

EC Council Directive 93/42/EEC on medical devices of 14 June 1993

Medical Devices Act MPG of 02 August 1994


DIN EN 60601-1

DIN EN 60601-1-2

DIN EN ISO 10993-1

HILOTHERM GmbH reserves the right to change specifications without notice.

### 7.4 Faults and troubleshooting

Error	Possible cause	Measures
Device without function, no display on the display	<ol style="list-style-type: none"> <li>1. Power failure</li> <li>2. Fuse defective</li> <li>3. Fuse repeatedly defective</li> <li>4. Power plug does not have a power plug Contact</li> <li>5. Device defective</li> </ol>	<ol style="list-style-type: none"> <li>1. Turn off the device</li> <li>2. Replace the fuse</li> <li>3. Customer Service</li> <li>4. Plug connection of the mains connection Check the line</li> <li>5. Customer Service</li> </ol>
Device does not cool	<ol style="list-style-type: none"> <li>1. Heat exchanger with dust Added</li> <li>2. Device defective</li> </ol>	<ol style="list-style-type: none"> <li>1. Heat exchanger carefully with Vacuum cleaner or soft brush clean.</li> <li>2. Customer Service</li> </ol>
Display Anzeige  Fast flashing snow symbol with exclamation mark The cooling water is outside the ideal temperature range for the application (too warm)	<ol style="list-style-type: none"> <li>1. Heat exchanger with dust Added</li> <li>2. Device defective</li> <li>3. Ambient temperature too high</li> </ol>	<ol style="list-style-type: none"> <li>1. Open the right-sided blue housing cover and carefully clean the heat exchanger with a vacuum cleaner or soft brush.</li> <li>2. Customer Service</li> <li>3. Operate the device in the specified temperature range</li> </ol> <p>Note: Cooling is still possible and should be continued</p>
No or too little water circulation	<ol style="list-style-type: none"> <li>1. Pump is not vented</li> <li>2. Hoses or cuff snapped off</li> <li>3. Clutch not engaged</li> <li>4. Pump defective</li> </ol>	<ol style="list-style-type: none"> <li>1. Venting, see section 3.3</li> <li>2. Eliminate the kink</li> <li>3. Press in clutches until they lock audibly</li> <li>4. Customer Service</li> </ol>
Display Display "E21"	<ol style="list-style-type: none"> <li>1. too little water in the tank</li> <li>2. Level sensor is fixed</li> </ol>	<ol style="list-style-type: none"> <li>1. Refill demineralized water</li> <li>2. Drain and fill repeatedly</li> </ol>
Display Display "E11"	Pumpe defect	1. Technischer Service
Display Display "E01"	Temperature difference between the two temperature sensors detected.	<ol style="list-style-type: none"> <li>1. Recalibration/Reset</li> <li>2. If 1 is not successful then inform Technical Service</li> </ol>
Display Display "E02"	Temperature sensors not connected / cable break	<ol style="list-style-type: none"> <li>1. . Recalibration/Reset</li> <li>2. If 1 is not successful then inform Technical Service</li> </ol>

Display Display <b>"E03"</b>	Temperature too low < 3°C	1. Recalibration / Reset 2. If 1 is not successful, check the ambient temperature Let the device warm up
Display Display <b>"E04"</b>	Temperature too high > 42°C	1. Recalibration 2. If 1 is not successful, check the ambient temperature. Allow the device to cool down
Display Display <b>"E05"</b>	Increased temperature difference between the two temperature sensors detected	1. . Recalibration/Reset 2. If 1 is not successful then inform Technical Service
Display Display <b>"E99"</b>	Control system defekt	1. Inform technical service
Plug connection of the hoses is difficult	1. O-ring is not greased 2. Plug connection is damaged	1. Easily grease the spout with petroleum jelly 2. Customer Service

**Attention: Opening the device leads to the loss of warranty claims!**


**Exception:** Right-sided blue housing cover for cleaning the heat exchanger

**Hint:**

In the event of an **E0x** temperature error , **resetting the temperature system settings can fix the problem.**  
**This reset is done by pressing all 3 buttons (up, down and enter) at the simultaneously switching on the device on the power switch of the back of the device.**  
**After the reset, turn the device off and on again on the power adapter**



**A successfully performed reset can be recognized by the fact that the operating hours on the start display are set to "0h".**

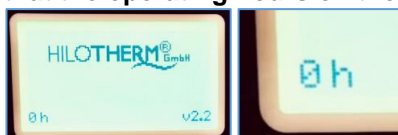

## 8. Accessories and spare parts

All spare parts and accessories are available from HILOTHERM GmbH or an authorized dealer.

### Accessories

Only original HILOTHERM accessories may be used.

**Caution:** The use of other devices or accessories in conjunction with the Hilotherapy device is not permitted.

Standard accessory list per device:

Number	Article	Designation
1	40000332	Power cord (C,F 230V 50 Hz)
2	40000259	Connection hose
1	40000379	Vent set

### Spares

Only original spare and wear parts guarantee device safety and reliability.

The replacement of parts may only be carried out by qualified persons.

The hilotherapy system is constantly evolving.

To ensure that you always receive the right spare part even after technical changes, we ask you to provide us with the following data with each order:

Designation: **Type HT 02Series**

number.....  
 Year of construction.....

## 9. Cuffs

### 9.1 Variants and material properties

For the Hilotherm ChemoCare System, the following cuffs are to be used for thermotherapeutic application in anatomically adapted form:

- Hand cuff
- Foot cuff slippers

#### Material properties:

Cuff film:	TPU (thermoplastic polyurethane) – latex-free, silicone-freeTuff
insulation	TPU foam
Hose insulation (for MM sleeves)	TPU foam
Hose:	TPU (thermoplastic polyurethane)
Closure grommet:	Brass, nickel-plated / POM

### 9.2 Warnings

- The cuffs may only be used in conjunction with the Hilotherapy device.
- The cuffs must not come into contact with chemicals containing benzene and phenol.
- Before each application of the cuff, it must be checked for integrity (no blistering, no leakage). Only intact cuffs are to be used. If abnormalities occur during treatment, such as blistering or leakage, the application should be discontinued immediately. In the event of defects in the hose and capillary system of the cuffs, these must be discarded.
- When handling the cuffs, care must be taken to ensure that they are not damaged by sharp objects.
- Care must be taken to ensure that the flow of the channels in the cuffs is not prevented by folding the cuffs or by pressing.
- When coupling and uncoupling the closure grommets of the hose system to the Hilotherapy device, a few drops of water may escape. It must be ensured that these do not get on wound dressings and bandages! The cuff may only be applied to intact skin or wound dressings.
- Water escaping due to any leaks usually does not pose any hygienic hazard to the user with a predetermined water change and regular maintenance and cleaning of the system.

### 9.3 Use of the product on the patient / intended purpose

The cuffs are used exclusively for external use.

The application to corresponding skin areas is carried out on wound dressings or directly on intact skin.

For repeated therapeutic use, we recommend the patient-related assignment of a cuff.

EM cuffs are intended for single use per patient and must not be reprocessed. With these EM cuffs, a yellow or blue-green coloration of the cuff material may occur when used over a longer period of time. This discoloration is material-related and does not pose any hygienic hazard to the user.

### 9.4 Risk classification of medical devices according to RKI

The risk assessment and assessment is based on the Federal Health Gazette 44 (2001): 1115-1126: Requirements for hygiene in the reprocessing of medical devices.

The operator is responsible for the implementation of the treatment measures by qualified personnel and with appropriate validated procedures.

The individual steps of the preparation must be adapted to

- the medical device
- processing

- the application on the patient.

The cuffs are intended only for contact with intact skin. Pathologically altered skin areas (e.B. abrasions, infectious wounds) or surgical wounds must be provided with a wound dressing before treatment.

With regard to the type of application of the cuffs and the resulting risk, they are classified as **uncritical medical** devices.

### 9.5 Application description

When coupling and uncoupling the closure grommets of the hose system to the Hilotherapy device, a few drops of water may escape. It must be ensured that these do not get on wound dressings and bandages!

The filled cuff is loosened without exerting pressure on the part of the body to be treated. Fixation measures may be necessary.

The duration of the treatment depends on the instructions of the attending physician.

### 9.6 Storage, storage and transport

The cuffs are delivered with low germs in a transport and dust protection bag and in an additional outer carton.

Storage must be dust-free, dry, without exposure to UV radiation and without temperature fluctuations at room temperature.

### 9.7 Disinfection, cleaning and

dryingCots, appliances and accessories are manufactured in a clean and hygienically harmless condition and delivered accordingly. **However**, the condition of the products mentioned in the delivery state cannot be specified as "sterile".

#### 9.7.1 Cuffs

Cuffs labelled as single patient use cannot be reprocessed and are intended only for use during treatment on a patient.

Disinfection may be required before applying the cuffs to wound dressings or to the part of the body to be treated, depending on the instructions of the attending physician.

#### Reprocessing / Duration of use

Cuffs that are not labeled as disposable can be cleaned, reprocessed and disinfected. This also applies to multiple sleeves that are provided with PU foam insulation on the outer surfaces.

With proper processing and depending on the frequency of use, multiple cuffs can be used over a period of about one year.

Due to frequent use of the multiple sleeves and the reprocessing process, the cuffs are subject to wear caused by the application. Wear-related defects and defects in the cuffs are not subject to any warranty claims

#### Cleaning and disinfection procedures

The manual cleaning and disinfection of the cuffs must be carried out after treatment on the patient with conventional and approved cleaning and surface disinfectants in the hospital area.

Corresponding information such as the list of approved disinfectants and recommendations for disinfection procedures can be found on the website of the Robert Koch Institute ([www.rki.de](http://www.rki.de))

Wipe disinfection is recommended for the smooth surfaces of the cuffs, and wipe or spray disinfection for surfaces with a material-like surface (blue insulation). Disinfection must be carried out by qualified personnel.

The cuffs as well as the insulation are made of polyurethane, this material is well tolerated with a variety of disinfectants. With regard to compatibility, concentration and exposure time of the disinfectant, the respective manufacturer's instructions must be observed.

If properly carried out, multi-cuffs can be reprocessed over a period of about one year.



A hygiene and disinfection plan with corresponding process descriptions and work instructions as part of the quality management must be drawn up by the operator in order to be able to document a comprehensible and validated treatment process.

### **Example of a mechanical cleaning and disinfection of non-critical medical devices**

Cleaning, disinfection, rinsing and drying is possible in a cleaning and disinfection machine with a validated chemical or chemical-thermal process at a maximum of 55 °C. The cuff must be fixed within the device chamber in suitable holders in such a way that the film surface can be easily rinsed by the cleaning and disinfection media. The procedure should be followed by automatic drying in the device. The application of the mechanical process must be carried out by qualified personnel in accordance with the specifications of the quality management (e.B. process description, work and procedure instructions) of the operator.

### **9.7.2 Basic device**

The surface of the devices consists mainly of ABS plastic and, if necessary, can be ideally treated by means of wipe disinfection after selecting a suitable method and disinfectant. A disinfection of the cooling circuit is not necessary if the maintenance specifications and regular water change are observed.

### **9.8 Control and testing**

After successful disinfection and cleaning, a visual inspection and inspection of the cuffs is required. If the cuff film, the hoses and / or the closure spouts are damaged, the cuff must be discarded. Before use on the patient, the cuff should be checked for tightness by connecting it to the Hilotherapy device and filling it.

### **9.9 Sterilization**

The cuffs cannot be sterilized.

## 10. Annex

### A Guidelines and manufacturer's declaration

#### A1

Table 1 (EN 60601-1-2)

<b>Guidelines and manufacturer's declaration - Electromagnetic emissions</b>			
The Hilotherm Chemocare is designed to operate in an electromagnetic environment as specified below . The customer or user of The Hilotherm Chemocare should ensure that it operates in such an environment.			
<b>Emission measurements</b>	<b>Agreement</b>	<b>Electromagnetic Environment Guide</b>	
RF mailings to CISPR 11	Group 1	The Hilotherm Chemocare uses RF energy exclusively for its internal function. Therefore, its RF emission is very low and it is unlikely that neighboring electronic devices will be disturbed.	
RF mailings to CISPR 11	Class B	The Hilotherm Chemocare is suitable for use in all facilities, including those in the residential area and those directly connected to a public utility network that supplies buildings used for residential purposes.	
Transmission of harmonics according to IEC 61000-3-2	Class A		
Emission of voltage fluctuations/flicker according to IEC 61000-3-3	jibes		

#### A2

Table 2 (EN 60601-1-2)

<b>Guidelines and Manufacturer's Declaration - Electromagnetic Immunity</b>			
The Hilotherm Chemocare is designed to operate in the electromagnetic environment specified below. The client or user of the Hilotherapy system should ensure that it is used in such an environment.			
<b>Immunity tests</b>	<b>IEC 60601 - Test level</b>	<b>Match tuning level</b>	<b>Electromagnetic Environment - Guidelines</b>
Discharge of static electricity (ESD) according to IEC 61000-4-2	± 6 kV contact discharge ± 8kV air discharge	± 6 kV Contact discharge ± 8 kV air discharge	Floors should be made of wood or concrete or provided with ceramic tiles. If the floor is provided with synthetic material, the relative humidity must be at least 30%.
Fast transient electrical disturbances/bursts according to IEC 61000-4-4	± 2 kV for mains cables ± 1 kV for input and output lines	± 2 kV for power lines not applicable	The quality of the supply voltage should match that of a typical business or hospital environment.
Surges according to IEC 61000-4-5	± 1 kV outer conductor outer conductor ± 2 kV outer conductor earth	± 1 kV outer conductor outer conductor ± 2 kV outer conductor earth	The quality of the supply voltage should match that of a typical business or hospital environment.
Voltage breaks, short conductor	< 5% UT	0% UT	The quality of the supply voltage should match that of a

<p>interruptions and fluctuations of the supply voltage according to IEC 61000-4-11</p>	<p>(&gt;95% drop in <math>U_T</math>) for 1/2period  40% <math>U_T</math> (60% drop in <math>U_T</math>) for 5 periods  70% <math>U_T</math> (30% slump in <math>U_T</math>) for 25 periods  5% <math>U_T</math> (95% drop in <math>U_T</math>) for 5s</p>	<p>40% <math>U_T</math>  70% <math>U_T</math>  5000 mS</p>	<p>typical business or hospital environment. If the user of the Hilotherm Chemocare requests continued function even in the event of interruptions in the power supply, it is recommended to <b>feed the Hilotherm Chemocare</b> from an uninterruptible power supply or a battery.</p>
<p>Magnetic field at the supply frequency (50/60 Hz) according to IEC 61000-4-8</p>	<p>3 A/m</p>	<p>3 A/m</p>	<p>Magnetic fields at the mains frequency should correspond to the typical values found in the business and hospital environment.</p>
<p>Note: <math>U_T</math> is the AC mains voltage before applying the test levels.</p>			

**A3**

Table 4 (EN 60601-1-2)

**Guidelines and Manufacturer's Statement - Electromagnetic immunity for ME equipment or ME systems that are not life-sustaining.**

The Hilotherm Chemocare is designed to operate in the electromagnetic environment specified below. The client or user of the Hilotherapy system should ensure that it is used in such an environment.

Immunity tests	IEC 60601 - Test level	Conformity level	Electromagnetic Environmental Guidelines
<p>Conducted RF disturbances according to IEC 61000-4-6</p> <p>Radiated RF disturbances according to IEC 61000-4-3</p>	<p>3 V EFFECTIVE value 150 kHz to 80 MHz</p> <p>3 V/m 80 MHz to 2.5 GHz</p>	<p>U1 = 3 V</p> <p>E1 = 3 V/m</p>	<p>Portable and mobile radios should be available at no shorter distance from the Hilotherm Chemocare including the cables can be used as the recommended protective distance, which is calculated according to the equation applicable to the transmission frequency.</p> <p><b>Recommended protective distance:</b></p> $d = \frac{3,5}{V1} \sqrt{P}$ $d = \text{[]for 80 MHz to 800 MHz } \frac{3,5}{E1} \sqrt{P}$ $d = \text{[]for 80 MHz to 800 MHz } \frac{7}{E1} \sqrt{P}$ <p>with P as the rated power of the transmitter in watts (W) as specified by the transmitter manufacturer and d as the recommended protective distance in meters (m).</p> <p>The field strength of stationary radio transmitters should be lower than the compliance level at all frequencies according to an on-site investigation.</p> <p>Interference is possible in the vicinity of devices bearing the following figurative sign.</p>

Note 1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note 2: These guidelines may not be applicable in all cases. The propagation of electromagnetic quantities is influenced by absorptions and reflections of buildings, objects and people.

a) The field strength of stationary transmitters, such as .B base stations of radio telephones and mobile land radios, amateur radio stations, AM and FM radio and television stations cannot theoretically be precisely predetermined. In order to determine the electromagnetic environment with regard to the stationary transmitters, a study of the site should be considered. If the measured field strength at the site where the hilotherapy system is used exceeds the above compliance levels, the hilotherapy system should be observed to demonstrate its intended function. If unusual performance characteristics are observed, additional measures may be required, such as .B a change in orientation or a different location of the hilotherapy system.

b) Over the frequency range from 150 kHz to 80 MHz, the field strength should be less than [v1] V/m.

**A4**

Table 6 (EN 60601-1-2)

<b>Recommended protection distances between portable and mobile RF telecommunications equipment and the ME device or ME system for ME devices or ME systems that are not life-sustaining.</b>			
The Hilotherm Chemocare is designed to operate in an electromagnetic environment where RF disturbances are controlled. The customer or user of the Hilotherm Chemocare can help to avoid electromagnetic interference by maintaining the minimum distance between portable and mobile RF telecommunications equipment (transmitters) and the Hilotherm Chemocare, depending on the output power of the communication device, as specified below.			
<b>Rated power of the transmitter W</b>	<b>Protective distance depending on the transmission frequency m</b>		
	150 kHz to 80 MHz $d = \frac{3,5}{V1} \sqrt{P}$	80 MHz to 800 MHz $d = \frac{3,5}{E1} \sqrt{P}$	800 MHz to 2.5 GHz $d = \frac{7}{E1} \sqrt{P}$
0,01	0,12	0,12	0,23
0,1	0,37	0,37	0,74
1	1,17	1,17	2,33
10	3,70	3,70	7,37
100	11,70	11,70	23,33
For transmitters whose maximum rated power is not specified in the table above, the recommended protective distance d in meters (m) can be determined using the equation belonging to the respective column, where P is the maximum rated power of the transmitter in watts (W) as specified by the transmitter manufacturer.			
Note 1: At 80 MHz and 800 MHz, the higher frequency range applies.			
Note 2: These guidelines may not be applicable in all cases. The propagation of electromagnetic quantities is influenced by absorptions and reflections of buildings, objects and people.			

**HILOTHERM®**

Wittumweg 38, D-88260 Argenbühl-Eisenharz

**EG-Konformitätserklärung für Medizinprodukte  
(Anhang II.3 (ohne II.4) MDD)  
EC-Declaration of Conformity (Annex II.3 (without II.4) MDD)**

Hiermit erklären wir  
*We, the undersigned*

Hilotherm GmbH  
Wittumweg 38  
D-88260 Argenbühl-Eisenharz

In eigener Verantwortung, dass nachstehendes Medizinprodukt  
*Declare on our own authority that the referred medical device below*

Produktgruppe / <i>Product Group</i>	Thermotherapie System / <i>Thermotherapy system</i>
Produktbezeichnung / <i>Product Name</i>	HILOTHERM ChemoCare / <i>HILOTHERM ChemoCare</i>
Produkttyp / <i>Product Type</i> :	HT02 / <i>HT02</i>
Klassifizierung nach MDD / <i>Classification accoring MDD</i>	Klasse IIa / <i>Class IIa</i>

den grundlegenden Anforderungen der nachfolgenden Richtlinie entsprechen  
*comply with the essential requirements of the following directive*

**Medizinprodukte Richtlinien 93/42/EWG  
*Medical Device Directive 93/42/EC***

Gekennzeichnet durch  
*marked with*

**CE 0123**

Benannte Stelle / *Notified body*:  
TÜV SÜD Product Service GmbH  
Ridlerstraße 65  
D-80339 München

Hilotherm bestätigt ebenfalls das Einhalten folgender Richtlinie  
*Hilotherm also confirms the compliance to following directive*

**RoHS II**

Diese Konformitätserklärung hat Gültigkeit bis zur Änderung geschriebener Inhalte dieser Erklärung  
*The declaration is valid until the change of any contend of the declaration*

Eisenharz, 2021-01-14



ppa. Klaus Janisch